



Run the Iris X80 Configuration Assistant, connect the Iris X80 and click Ready. After selecting your software, Click Ready on the right.

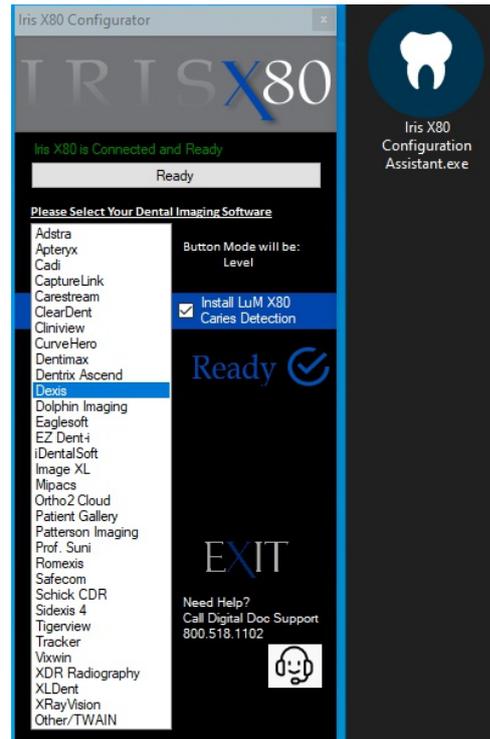

After selecting a patient in Dexis, Click on the Dexis Banner, then select Preferences.

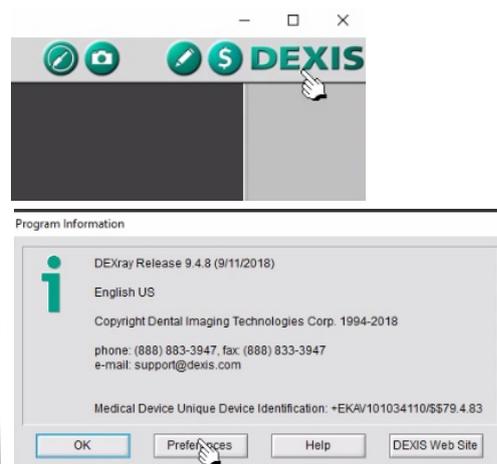

Select Video Acquisition from the left panel, Modify the settings on the right panel to match the provided screenshot.

