



Run the Iris X80 Configuration Assistant, connect the Iris X80 and click Ready. After selecting your software, Click Ready on the right.

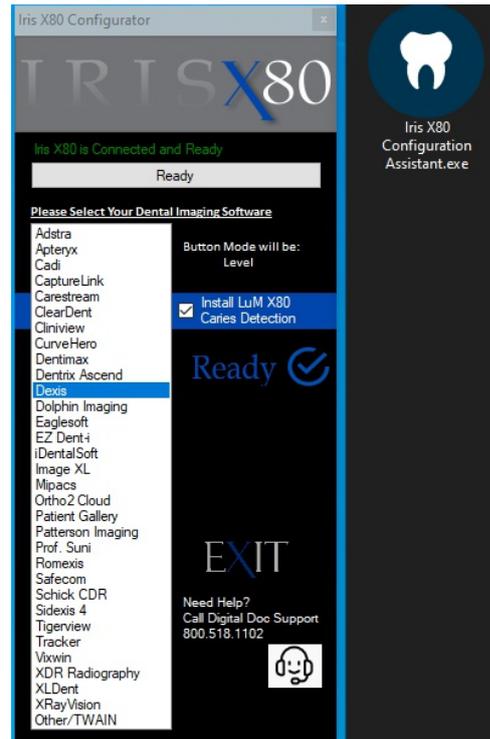

After selecting a patient in Dexis, Click on the Dexis Banner, then select Preferences.

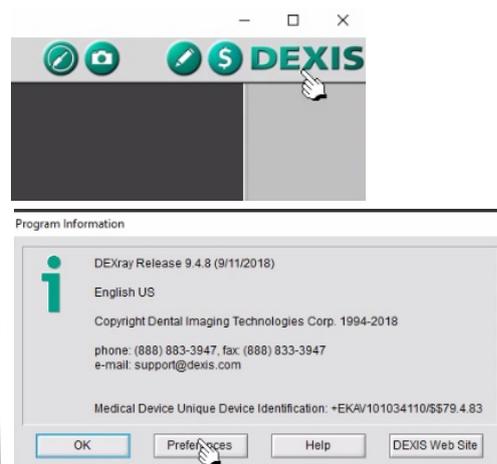

Modify the settings to match the table below. Capture Device will need to be 'automatic' until you have launched video with the camera, then you may go back

